

## INTENDED USE

The Mouse Anti-Tetanus Toxoid IgG ELISA Kit detects and quantifies tetanus toxoid/toxin-specific IgG in mouse serum or plasma of vaccinated or immunized animals. This immunoassay is suitable for:

- Determining immune status relative to non-immune controls;
- Assessing efficacy of vaccines, including dosage, adjuvantcy, route of immunization and timing;
- Qualifying and/or standardizing vaccine batches and protocols.

## GENERAL INFORMATION

Tetanus, a neurotoxic disease resulting in severe muscular spasm, is caused by *Clostridium tetani* bacteria. Tetanus toxin, a protein exotoxin produced only by *C. tetani*, is central to tetanus pathogenesis. Vaccination with the inactivated toxin (toxoid) elicits high levels of protection from the disease. The toxoid also acts as an adjuvant to boost immune responses to other antigens when combined in a vaccine, either mixed or covalently conjugated. Vaccines for tetanus are available in combination with other vaccines, e.g., pertussis, diphtheria, H. influenza b, hepatitis & polio.

Monitoring the efficacy of vaccines by determining the anti-tetanus levels in the host, including for clinical trials using new formulation of vaccines, is often required. The ADI Anti-Tetanus Toxoid ELISAs will quantify antibodies produced by vaccines as well as from infection with the toxin-producing organisms.

## PRINCIPLE OF THE TEST

The Mouse Anti-Tetanus Toxoid IgG ELISA kit is based on the binding of mouse anti-tetanus toxoid IgG in samples to tetanus toxoid immobilized on the microwells, and anti-tetanus toxoid antibody is detected by anti-mouse IgG-specific antibody conjugated to HRP (horseradish peroxidase) enzyme. After a washing step, chromogenic substrate (TMB) is added and color is developed by the enzymatic reaction of HRP on the substrate, which is directly proportional to the amount of anti-tetanus toxoid IgG present in the sample. Stopping Solution is added to terminate the reaction, and absorbance at 450nm is then measured using an ELISA microwell reader. The activity of mouse IgG antibody in samples is calculated relative to anti-tetanus toxoid calibrators.

## PRODUCT SPECIFICATIONS

### Specificity

Purified tetanus toxoid is used to coat the microwells; thus the assay is specific for antibodies directed to tetanus toxoid or toxin. The anti-Mouse IgG HRP conjugate reacts with mouse IgG antibodies that bind to toxoid on the plate; IgA, IgM and IgE antibody would not be measured above background signals.

### Assay Sensitivity

The tetanus toxoid coating level, HRP conjugate concentration and Low NSB Sample Diluent are optimized to differentiate anti-tetanus toxoid IgG from background (non-antibody) signal with mouse serum samples diluted 1:100.

### Calibrator Values

The calibrators are dilutions of antibody reactive to tetanus toxoid. Values are assigned as arbitrary anti-tetanus toxoid activity units.

## KIT CONTENTS

The microtiter well plate and all other reagents, if unopened, are stable at 2-8°C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

**To Be Reconstituted:** Store as indicated.

Component	Preparation Instructions
<b>Wash Solution Concentrate (100x)</b> Cat. No. WB-100, 10ml	Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Wash Solution</b> and store at ambient temperature until kit is used entirely.
<b>Sample Diluent Concentrate (20x)</b> Cat. No. SD-20T, 10ml	Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Sample/Conjugate Diluent</b> and store at 2-8°C until the kit lot expires or is used up.
<b>Anti-Mouse IgG- HRP Conjugate Concentrate (100x)</b> Part H-MsG.211, 0.15ml	Peroxidase conjugated anti-mouse IgG in buffer with protein, detergents and antimicrobial as stabilizers. Dilute fresh as needed; 10ul of concentrate to 1ml of <b>Working Sample/Conjugate Diluent</b> is sufficient for 1 8-well strip. Use within the working day and discard. Return 100X to 2-8°C storage.

**Ready For Use:** Store as indicated on labels.

Component	Part	Amt	Contents
<b>Tetanus Toxoid Microwell Strip Plate</b>	930-111	8-well strips (12)	Coated with tetanus toxoid, and post-coated with stabilizers.
<b>Anti-Tetanus Toxoid Calibrators</b>			
10 U/ml	930-212B	0.65 ml	Four (4) vials, each containing anti-tetanus toxoid IgG levels in arbitrary activity Units; diluted in buffer with protein, detergents and antimicrobial as stabilizers.
25 U/ml	930-212C	0.65 ml	
50 U/ml	930-212D	0.65 ml	
100 U/ml	930-212E	0.65 ml	
<b>Mouse Anti-Tetanus IgG Positive Control</b>	930-130PC	0.65 ml	Mouse x-tetanus toxoid IgG, in buffer with protein, detergents and antimicrobial. Value range on label.
<b>Low NSB Sample Diluent</b>	TBTm	30 ml	Buffer with protein, detergents and antimicrobial as stabilizers. Use as is for sample dilution. See <b>Assay Design</b> , page 3.
Reduces non-specific binding	<b>Not for HRP Conjugate dilution.</b>		
<b>TMB Substrate</b>	80091	12 ml	Chromogenic substrate for HRP containing TMB and peroxide.
<b>Stop Solution</b>	80101	12 ml	Dilute sulfuric acid.

Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml. A multi-channel pipettor is recommended.
- Disposable glass or plastic 5-15ml tubes for diluting samples and Anti-mouse IgG HRP Concentrate.
- Graduated cylinder to dilute Wash Concentrate; 0.2-1L.
- Stock bottle to store diluted Wash Solution; 200ml to 1L.
- Distilled or deionized water to dilute reagent concentrates.
- Microwell plate reader at 450 nm wavelength.

## PRECAUTIONS AND SAFETY INSTRUCTIONS

Calibrators, Sample Diluent, and Antibody HRP contain bromonitrodioxane (BND: 0.05%, w/v). Stop Solution contains dilute sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. MSDS for TMB, sulfuric acid and BND can be requested

## LIMITATIONS OF THE ASSAY

### Calibrator Curve Quantitation

To quantitate antibody activity from a calibrator curve (such as provided with the kit), the dilution curve of the samples must be parallel to the calibrator curve, to avoid different values being obtained from different regions of the curve. Antibodies that are not matched in tetanus avidity will often have non-parallel dilution curves. In these cases, antibody activity is best expressed as a titer relative to a reference positive such as the 25 U/ml Calibrator, or another Calibrator in the kit (see Calculation of Results).

## ASSAY DESIGN AND SET-UP

### Sample Collection and Handling

Culture medium, serum and other biological fluids may be used as samples with proper dilution to avoid solution matrix interference. For **serum**, collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. For other samples, including **tissue culture media**, clarify the sample by centrifugation and/or filtration prior to dilution in Sample Diluent.

### Antibody Stability

Initial dilution of serum into **Working Sample Diluent** (WSD) is recommended to stabilize antibody activity. This enhances reproducible sampling, and stabilizes the antibody activity for years, stored refrigerated or frozen. Further dilution into **Low NSB Sample Diluent** (LNSD), which provides the lowest assay background, should be at least 10 times the initial dilution and performed the same day as the assay.

Example: Initial (1/5): 10ul serum + 40ul WSD [or 0.1ml + 0.4ml]  
Further (1/50): 10ul initial (1/5) + 90ul LNSD (1/50)

### Assay Design

Review Calculation of Results (p5-7) and Limits of the Assay (above) before proceeding:

- **Select the proper sample dilutions.** Account for expected potency of positives and minimize non-specific binding (NSB) and other matrix effects; for example, non-immune samples should give net signal <0.5 OD. This is usually 1/100 or greater dilution for mouse sera with normal levels of IgG and IgM. Dilute samples in **Working Sample Diluent (1xSD20T)** or in **Low NSB Sample Diluent (TBTm)** (see above). Note: **all samples** must be diluted in the same diluent for proper comparison – either TBTm or 1xSD20T.
- Run a Sample Diluent **Blank**. This signal is an indicator of proper assay performance, especially of washing efficacy, and is used for net OD calculations, if required. Blank OD should be <0.3. See **Method A** and **B**.
- Run a set of Calibrators. Calibrators validate that the assay was performed to specifications, and can be used to normalize between-assay variation for enhanced precision. Reading values off a Calibrator curve, **Method C**, has limitations. See Limits of the Assay above.
- Run the Mouse Anti-Tetanus IgG **Positive Control**; net OD > **0.5**.
- Run samples in duplicate if used for quantitation; non-immunes that are significantly lower than immunes may be run in singlicate. The Calibrators that are used for quantitation, e.g., for between-assay normalization, should be run in duplicate. When determining titer from a dilution curve, singlicates can be run if more than two dilution points are used for titer calculations.

## Plate Set-up

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

- Determine the number of wells for the assay run. Duplicates are recommended, including 8 Calibrator wells and 2 wells for each sample and control to be assayed.
- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.
- Add 200-300ul Working Wash Solution to each well and let stand for about 5 minutes. Aspirate or dump the liquid and pat dry on a paper towel before sample addition.

## Assay Procedure

**ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE.** After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

### 1. 1<sup>st</sup> Incubation [100ul – 60 min; 4 washes]

- Add 100ul of calibrators, samples and controls each to pre-determined wells.
- Tap the plate gently to mix reagents and incubate for 60 minutes.
- Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer may be used. Improper washes may lead to falsely elevated signals and poor reproducibility.

### 2. 2<sup>nd</sup> Incubation [100ul – 30 min; 5 washes]

- Add 100ul of diluted Anti-mouse IgG HRP to each well.
- Incubate for 30 minutes.
- Wash wells 5 times as in step 2.

### 3. Substrate Incubation [100ul – 15 min]

- Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
- Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.

Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, or read OD at 405-410 nm (results are valid).

### 4. Stop Step [Stop: 100ul]

- Add 100ul of Stop Solution to each well.
- Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.

### 5. Absorbance Reading

- Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
- Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well background.

## INTERPRETATION OF RESULTS

### Calculation of Results

Consider several data reduction methods to best represent the relationships among experimental and control groups, to determine **Positive Immune** and **Negative Non-immune**, and to **Quantitate** positive antibody levels.

**Method A. Antibody Activity** [ELISA Signal & Sample Dilution]  
Represent data as net OD units (A450 signal; blank subtracted) ÷ dilution = **Total Activity Units**.

A Calibrator values in the mid-OD range (e.g., 25 U/ml) can be used to normalize inter-assay values.

### Method B. Positive Index

Experimental sample values may be expressed relative to the values of Control or Non-immune samples, by calculation of a **Positive Index**. One typical method is as follows:

1. Calculate the net OD mean + 2 SD of the Control/Non-immune samples = **Positive Index**.
2. Divide each sample net OD by the Positive Index. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

A sample value would be **Positive** if significantly above the value of the pre-immune serum sample or a suitably determined non-immune panel or pool of samples, tested at the same sample dilution. This calculation **quantifies** the positive Antibody Activity level.

### Example:

Sample	Assay Net OD		Calculation using Positive Index	
	Control	Exptl	Control	Exptl
1	0.243	2.358	0.49	<b>4.79</b>
2	0.351	0.597	0.71	<b>1.21</b>
3	0.286	1.421	0.58	<b>2.89</b>
4	0.357	1.268	0.73	<b>2.58</b>
5	0.512	0.857	<b>1.04</b>	<b>1.74</b>
6	0.342	1.296	0.70	<b>2.63</b>
7	0.298	0.608	0.61	<b>1.24</b>
8	0.285	0.369	0.58	0.75
9	0.157	0.864	0.32	<b>1.76</b>
10	0.187	0.543	0.38	<b>1.10</b>
Mean	0.302			
SD	0.095			
Mean +2 SD	<b>0.492</b>			<b>= Positive Index</b>

## CALCULATION OF RESULTS (continued)

### Method C. Use of a Calibrator Curve


When the dilution curves of samples are parallel to the Calibrator curve (see Limits of the Assay), the Anti-tetanus toxoid activity units may be determined by interpolation from the Calibrator curve. The results may be calculated using any immunoassay software package. If software is not available, Anti-tetanus toxoid activity concentrations may be determined as follows:

1. Calculate the mean OD of duplicate samples.
2. On graph paper plot the mean OD of the calibrators (y-axis) against the concentration (U/ml) of Anti-tetanus toxoid (x-axis). Draw the best fit curve through these points to construct the calibrator curve. A point-to-point construction is most common and reliable.
3. The Anti-tetanus toxoid activity concentrations in unknown samples and controls can be determined by interpolation from the calibrator curve.
4. Multiply the values obtained for the samples by the dilution factor of each sample.
5. Samples producing signals higher than the 80 U/ml calibrator should be further diluted and re-assayed.

### Typical Results:

Wells	Calibrators & Samples	A450 nm
A1,2	<b>Negative - Diluent Blank</b>	0.08
B1,2	10 U/ml <b>Calibrator</b>	0.45
C1,2	25 U/ml <b>Calibrator</b>	1.02
D1,2	50 U/ml <b>Calibrator</b>	1.87
E1,2	100 U/ml <b>Calibrator</b>	2.59
F1,2	<b>Sample, 1/100</b>	1.34

Sample:  $33 \times 100 = 3.3$  kU/ml

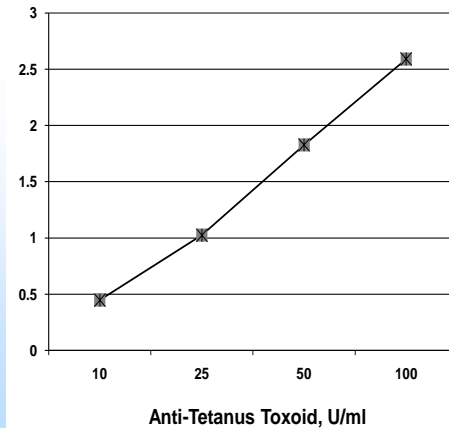

## CALCULATION OF RESULTS (continued)

### Method D. Titers from Sample Dilution Curves

The titer of antibody activity calculated from a dilution curve of each sample is recommended as the most accurate quantitative method. Best precision can be obtained using the following guidelines:


1. Use an OD value Index in the mid-range of the assay (2.0 – 0.5 OD); this provides the best sensitivity and reproducibility for comparing experimental groups and replicates. An arbitrary 1.0 OD is commonly used.
2. Prepare serial dilutions of each sample to provide a series that will produce signals higher and lower than the selected index. With accurate diluting, duplicates may not be required if at least 4 dilutions are run per sample.
3. A 5-fold dilution scheme is useful to efficiently cover a wide range which produces ODs both above and below 1.0 OD. The dilution scheme can be tightened to 3-fold or 2-fold for more precise comparative data.
4. A Calibrator value in the mid-OD range (e.g., 25 U/ml) can be used to normalize inter-assay values.

### Calculations

1. On a log scale of inverse of Sample Dilution as the x-axis, plot the OD values of the two dilutions of each positive sample having ODs above and below the OD value of the Index (arbitrary or selected Calibrator).
2. From a point-to-point line drawn between the two sample ODs, read the dilution value (x-axis) corresponding to the OD of the selected Index  
**= IgG Antibody Activity Units**

### Example:

II. A 1.0 OD Index was used to determine titer of 4 antibodies.

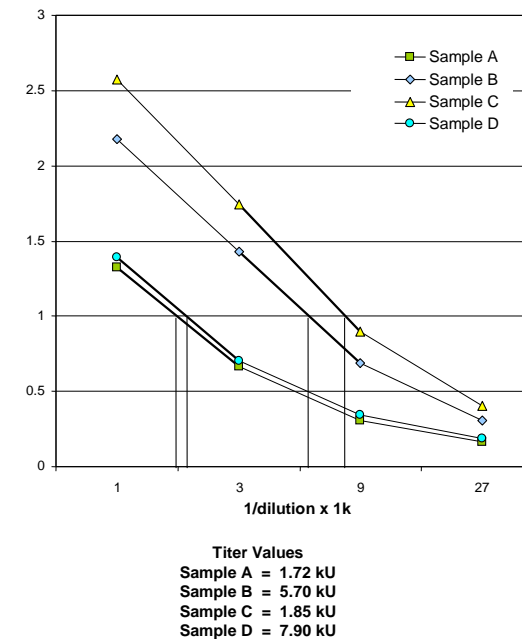

Instruction Manual No. M-930-130-TMG

# Mouse Anti-Tetanus Toxoid IgG ELISA Kit

Cat. No. 930-130-TMG, 96 tests

**For Quantitation of anti-Tetanus Toxoid/Toxin IgG in Serum/Plasma**

*For research use only, not for diagnostic or therapeutic use.*



**ALPHA DIAGNOSTIC INTERNATIONAL**

India Contact:

**Life Technologies™**  
Your Molecular & Cell Technology Partner

**Life Technologies (India) Pvt. Ltd.**  
306, Aggarwal City Mall, Opposite M2K Pitampura, Delhi – 110034 (INDIA).  
Ph: +91-11-42208000, 42208111, 42208222  
Mobile: +91-9810521400  
Fax: +91-11-42208444  
Email: customerservice@lifetechindia.com  
Web: www.lifetechindia.com

ELISA Kit Components	Amount	Part
Tetanus Toxoid Coated Microwell Strip Plate	8-well strips (12)	930-111
Mouse Anti-Tetanus IgG Positive Control	0.65 ml	930130PC
Anti-Tetanus Calibrator 10 U/ml	0.65 ml	930-212B
Anti-Tetanus Calibrator 25 U/ml	0.65 ml	930-212C
Anti-Tetanus Calibrator 50 U/ml	0.65 ml	930-212D
Anti-Tetanus Calibrator 100 U/ml	0.65 ml	930-212E
Anti-Mouse IgG HRP Conjugate (100X)	0.15 ml	H-MSG.211
Sample Diluent Concentrate (20x)	10 ml	SD20T
Low NSB Sample Diluent	30 ml	TBTm
Wash Solution Concentrate (100X)	10 ml	WB-100
TMB Substrate	12 ml	80091
Stop Solution	12 ml	80101
Product Manual	1 ea	M-930-130-TMG