

Human Cytochrome P450 2D6 (CYP2D6) ELISA Kit

to determine Human Cytochrome P450 2D6 (CYP2D6) in Serum, Blood Plasma, Saliva, Urine, Tissue Liquid Samples or related Biological Solutions.

INSTRUCTION MANUAL

FOR ELISA KIT No: L_{Tu}H2803EA



Life Technologies (India) Pvt. Ltd.

306, Aggarwal City Mall, Road No.44,

Pitampura, Delhi-110034, India

Toll Free: 1800-120-2434

Mobile: +91-98105-21400 | Fax: +91-11-42208444

customerservice@lifetechindia.com

INTENDED USE

This kit is used to determine Human Cytochrome P450 2D6 (CYP2D6) in the sample of serum, blood plasma, saliva, urine, tissue liquid samples or related biological solutions. For *in vitro* use only.

MANUAL VERSION 1.02

INTRODUCTION

ASSAY PRINCIPLE

Cytochrome P450 2D6 (CYP2D6), a member of the cytochrome P450 mixed-function oxidase system, is one of the most important enzymes involved in the metabolism of xenobiotics in the body. Whilst CYP2D6 is involved in the oxidation of a wide range of substrates of all the CYPs, there is considerable variability in its expression in the liver. The gene is located near two cytochrome P450 pseudogenes on chromosome 22q13.1. Alternatively, spliced transcript variants encoding different isoforms have been found for this gene. CYP2D6 activity was tested in "healthy infants receiving an oral dose (0.3 mg/kg) of dextromethorphan (DM) at 0.5, 1, 2, 4, 6, and 12 months of age. DM and its major metabolites were measured in urine. CYP2D6 genotype was determined by polymerase chain reaction-restriction fragment length polymorphism. This Human Cytochrome P450 2D6 (CYP2D6) ELISA Kit employs a two-site sandwich ELISA to quantitate CYP2D6 in samples. An antibody specific for CYP2D6 has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any CYP2D6 present is bound by the immobilized antibody. After removing any unbound substances, a biotin-conjugated antibody specific for CYP2D6 is added to the wells. After washing, Streptavidin conjugated Horseradish Peroxidase (HRP) is added to the wells. Following a wash to remove any unbound avidin-enzyme reagent, a substrate solution is added to the wells and color develops in proportion to the amount of CYP2D6 bound in the initial step. The color development is stopped and the intensity of the color is measured.

CHARACTERISTICS

-This Kit allows for the determination of CYP2D6 concentrations in Human serum, cell culture supernates and other biological fluids.

-Detection range: 2.5pg/mL-40pg/mL.

-The minimum detectable dose (MDD) of Human CYP2D6 is typically less than 0.1 pg/mL.

-Four samples of known concentration were tested twenty times on one plate to assess intra-assay precision. The CV (%) < 9%.

-Three samples of known concentration were tested in twenty separate assays to assess inter-assay precision. Assays were performed by at least three technicians using two lots of components. The CV (%) < 11%.

-To assess linearity of the assay, samples containing and/or spiked with high concentrations of Human CYP2D6 were diluted with the appropriate calibrator diluent to produce samples with values within the dynamic range of the assay. Linear regression analysis of samples versus the expected concentration yielded a correlation coefficient of 0.99.

-Human Cytochrome P450 2D6 (CYP2D6) ELISA Kit has high sensitivity and excellent specificity for detection of Human CYP2D6. No significant cross-reactivity or interference between Human CYP2D6 and analogues was observed.

PRODUCT INFORMATION

MATERIALS SUPPLIED AND STORAGE CONDITIONS

Store kit reagents at 2-8 °C for 6 months. Immediately after use remaining reagents should be returned to cold storage at 4 °C.

components	48T	96T	Storage conditions
Human CYP2D6 microplate	48 wells	96 wells	2-8 °C ¹
Human CYP2D6 standard	0.5 mL	0.5 mL	2-8 °C
HRP-Conjugated Human CYP2D6 detection antibody	3 mL	6 mL	2-8 °C
Standard diluent	1.5 mL	1.5 mL	2-8 °C
Sample diluent	3 mL	6 mL	2-8 °C
Chromogen solution A	3 mL	6 mL	2-8 °C
Chromogen solution B	3 mL	6 mL	2-8 °C
Stop solution	3 mL	6 mL	2-8 °C
Wash buffer	20 mL (20×)	20 mL (30×)	2-8 °C
Plate covers	1	2	RT
Booklet	1	1	RT

¹Return unused wells to the foil pouch containing the desiccant pack. Reseal along entire edge of the zip-seal.

May be stored for up to 1 month at 2-8 °C.

MATERIALS REQUIRED BUT NOT SUPPLIED

- 37 °C incubator
- Microplate reader
- Precision pipettes and tips
- Distilled water
- Disposable tubes for sample dilution
- Absorbent paper

ASSAY PROTOCOL

SAMPLE COLLECTION AND STORAGE

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

Tissue homogenates - For general information, hemolysis blood may affect the result, so you should rinse the tissues with ice-cold PBS (0.01M, pH=7.4) to remove excess blood thoroughly. Tissue pieces should be weighed and then minced

to small pieces which will be homogenized in PBS with a glass homogenizer on ice. (The volume depends on the weight of the tissue, 9mL PBS would be appropriate to 1 gram tissue pieces. Some protease inhibitor is recommended to add into the PBS.) To further break the cells, you can sonicate the suspension with an ultrasonic cell disrupter or subject it to freeze-thaw cycles. The homogenates are then centrifugated for 5 minutes at 5000×g to collect the supernate.

Cell culture supernatants and other biological fluids - Centrifuge samples for 20 minutes at 1000×g. Remove particulates and assay immediately or store samples in aliquot at -20 °C or -80 °C for later use. Avoid repeated freeze/thaw cycles.

Serum - Use a serum separator tube and allow samples to clot for two hours at room temperature or overnight at 4 °C before centrifugation for 20 minutes at approximately 1000×g. Assay freshly prepared serum immediately or store samples in aliquot at -20 °C or -80 °C for later use. Avoid repeated freeze/thaw cycles.

Plasma - Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge samples for 15 minutes at 1000×g at 2-8 °C within 30 minutes of collection. Remove plasma and assay immediately or store samples in aliquot at -20 °C or -80 °C for later use. Avoid repeated freeze/thaw cycles.

Note: Samples should be centrifuged adequately and no hemolysis or granule was allowed.

REAGENT PREPARATION

Bring all reagents to room temperature before use. If crystals have formed in the Buffer Concentrates, warm them gently until they completely dissolved.

Wash buffer - Dilute with Distilled or deionized water 1:30.


Sample dilution - If your samples need to be diluted, Deionized or distilled water is used for dilution of samples.

Standard - Pipette 150 µl of Standard Diluent into each tube. Use the stock solution to produce a 2-fold dilution series (below). Mix each tube thoroughly before the next transfer. The undiluted Standard serves as the high standard. Standard Diluent serves as the zero standard.

ASSAY PROCEDURE

1. Dilution of standard solution: This kit contains a standard of known concentration, which could be diluted in small tubes by the end-user by following the instruction in the table below:

40 pg/mL	Standard No.5	150µl High Standard + 150µl Standard diluent
20 pg/mL	Standard No.4	150µl Standard No.5 + 150µl Standard diluent
10 pg/mL	Standard No.3	150µl Standard No.4 + 150µl Standard diluent
5 pg/mL	Standard No.2	150µl Standard No.3 + 150µl Standard diluent
2.5 pg/mL	Standard No.1	150µl Standard No.2 + 150µl Standard diluent

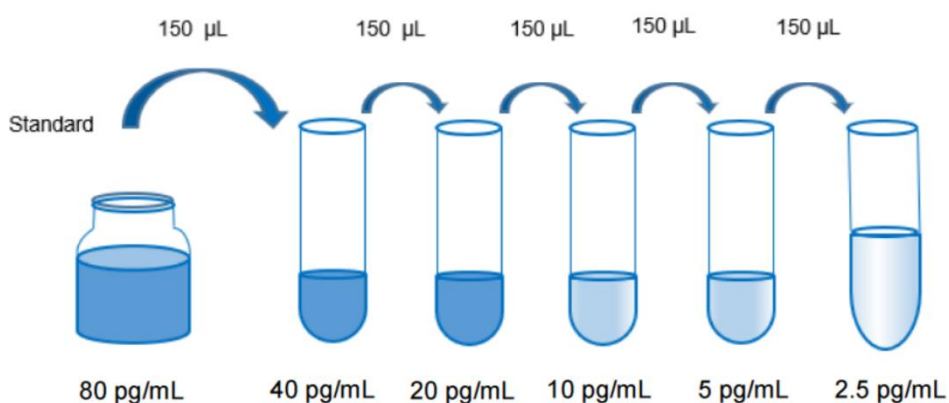

1. Prepare all reagents before starting assay procedure. It is recommended that all Standards and Samples be added in duplicate to the microplate.

2. Add standard: Set Standard wells, testing sample wells. Add diluted standard 50µl to standard well.
3. Add Sample: Add sample diluent 40 µl to testing sample well. Then add sample 10µl to testing sample well; for Blank well don't add anything.
4. Cover with a plate cover and incubate for 45 minutes at 37 °C.
5. Aspirate each well and wash, repeating the process four times for a total of five washes. Wash by filling each well with Wash buffer (250 µl) using a squirt bottle, manifold dispenser or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 50 µl HRP-Conjugate to each well, except blank well.
7. Cover with a new adhesive strip. Incubate for 30 minutes at 37 °C.
8. Repeat the aspiration/wash process for five times as in step 5.
9. Add 50 µl chromogen solution A and 50 µl chromogen solution B to each well. Gently mix and incubate for 15 minutes at 37°C. Protect from light.
10. Add 50µl Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green or the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
11. Read the Optical Density (O.D.) at 450 nm using a microtiter plate reader within 15 minutes.

CALCULATION

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density (O.D.). Create a standard curve by

reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration for each standard on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the Human CYP2D6 concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor (e.g. it is 5 in this case).

PRECAUTIONS

1. Do not mix or substitute reagents with those from other lots or sources.
2. This assay is designed to eliminate interference by other factors present in biological samples. Until all factors have been tested in the ELISA Immunoassay, the possibility of interference cannot be excluded.
3. Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.
4. When mixing or reconstituting protein solutions, always avoid foaming.
5. To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
6. To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
7. When using an automated plate washer, adding a 30 second soak period following the addition of Wash Buffer, and/or rotating the plate 180 degrees

between wash steps may improve assay precision.

8. Chromogen Solution is easily contaminated. If bluish prior to use, do not use.
9. Stop Solution should be added to the plate in the same order as the Chromogen solution. The color developed in the wells will turn from blue to yellow upon addition of the Stop Solution. Wells that are green in color indicate that the Stop Solution has not mixed thoroughly with the Chromogen solution.
10. Serum and plasma should be handled as potentially hazardous and capable of transmitting disease. Disposable gloves must be worn during the assay procedure, since no known test method can offer complete assurance that products derived from blood will not transmit infectious agents. Therefore, all blood derivatives should be considered potentially infectious and good laboratory practices should be followed.
11. All samples should be disposed of in a manner that will inactivate viruses.
12. Liquid Waste: Add sodium hypochlorite to a final concentration of 1.0%.
The waste should be allowed to stand for a minimum of 30 minutes to inactivate the viruses before disposal.

VALIDITY & STORAGE: 12 months (at 2-8°C, unopened).