

### Importance of 2,4-D Determination

2,4-D is a phenoxy herbicide used in the control of broadleaf weeds. It is one of the most widely used herbicides in the world. In the United States alone, approximately 46 million pounds are used each year. 2,4-D is a selective herbicide, affecting broadleaf weeds but not grasses, making it ideal for use in both agricultural (cereal grain crops) and non-agricultural settings (residential lawns, along roadways, and in aquatic weed control in and around lakes).

Humans may be exposed to 2,4-D through direct physical contact with treated plants or water sources or thorough ingestion of contaminated foods or drinking water. Drinking water sources can be contaminated through run-off (surface water) or leaching (ground water). 2,4-D has been found in surface waters across the U.S. The U.S. EPA lists 2,4-D as a compound which is likely to leach from soil and it has been found in groundwater in the U.S. as well as in Canada. Human exposure to 2,4-D can cause liver toxicity at low doses, producing inflammation, jaundice, and even acute hepatitis. Golfers exposed to 2,4-D have shown permanent liver damage leading to cirrhosis. Damage may also occur to the kidneys and adrenals, ovaries, testes, and thyroid. 2,4-D can cause neurotoxicity and has been linked to an increased risk of amyotrophic lateral sclerosis (ALS, also known as Lou Gehrig's Disease).

The EPA, under the Safe Drinking Water Act, has established a maximum contaminant level (MCL) of 70 ppb in drinking water. The World Health Organization has established an Acceptable Daily Intake (ADI) of 0.01 mg/kg of body weight.

The 2,4-D ELISA allows for the analysis of 41 samples in duplicate determination. Less than 1 mL of sample is required. The test can be performed in less than 2 hours.

### Performance Data


**Test sensitivity:** The limit of quantitation for 2,4-D (90% B/B<sub>0</sub> calculated from the average of 28 calibration curves) is approximately 1.67 ng/mL. The middle of the test (50% B/B<sub>0</sub> calculated from the average of 28 calibration curves) is approximately 13.71 ng/mL. Determinations closer to the middle of the calibration curve give the most accurate results.

**Test reproducibility:** Coefficients of variation (CVs) for standards: <10%; CVs for samples: <15%.

**Specificity:** Cross-reactivity of the Abraxis 2,4-D ELISA for related herbicides:

2,4-D	100%
2,4,5-T	66%
2,4-D isopropyl ester	57%
2,4-D methyl ester	56%
2,4-DB butyl ester	26%
MCPA	13%
2,4-DB	2.5%
Dichlorprop	1.2%
2,4,5-TP	< 0.1%

**Standard Curve:**

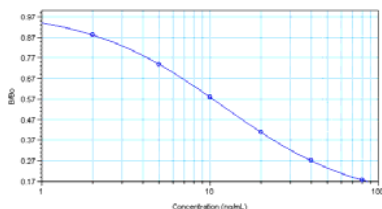

For demonstration purposes only. Not for use in sample interpretation.

**General Limited Warranty:** Abraxis LLC warrants the products manufactured by the Company, against defects and workmanship when used in accordance with the applicable instructions for a period not to extend beyond the product's printed expiration date. **Abraxis makes no other warranty, expressed or implied. There is no warranty of merchantability or fitness for a particular purpose**

For ordering or technical assistance contact:

**India Contact:**

**Life Technologies (India) Pvt. Ltd.**

306, Aggarwal City Mall, Road No. 44, Pitampura, Delhi – 110034, India

Mobile: +91-98105-21400, Tel: +91-11-42208000, 8111, 8222, Fax: +91-11-42208444

Email: customerservice@lifetechindia.com, www.atzlabs.com; www.lifetechindia.com

## 2,4-D ELISA (Microtiter Plate)

Enzyme-Linked Immunosorbent Assay for the Determination of 2,4-D in Water Samples

Product No. 54003A

### 1. General Description

The Abraxis 2,4-D ELISA is an immunoassay for the quantitative and sensitive screening of 2,4-D. This test is suitable for the quantitative and/or qualitative screening of 2,4-D in water samples. Samples requiring regulatory action should be confirmed by HPLC, GC/MS, or other conventional methods.

### 2. Safety Instructions

The standard solutions in the test kit contain small amounts of 2,4-D. In addition, the substrate solution contains tetramethylbenzidine and the stop solution contains diluted sulfuric acid. Avoid contact of stopping solution with skin and mucous membranes. If these reagents come in contact with skin, wash with water.

### 3. Storage and Stability

The 2,4-D ELISA should be stored in the refrigerator (4–8°C). The solutions must be allowed to reach room temperature (20-25°C) before use. Reagents may be used until the expiration date on the box.

### 4. Test Principle

The test is a direct competitive ELISA based on the recognition of 2,4-D by specific antibodies. 2,4-D, when present in a sample, and a 2,4-D-HRP analogue compete for the binding sites of the mouse anti-2,4-D antibodies in solution. The 2,4-D antibodies are then bound by a second antibody (goat anti-mouse) immobilized on the wells of the microtiter plate. After a washing step and addition of the substrate solution, a color signal is generated. The intensity of the blue color is inversely proportional to the concentration of 2,4-D present in the sample. The color reaction is stopped after a specified time and the color is evaluated using an ELISA reader. The concentrations of the samples are determined by interpolation using the standard curve constructed with each run.

### 5. Limitations of the 2,4-D ELISA, Possible Test Interference

Although many organic and inorganic compounds commonly found in samples have been tested and found not to interfere with this test, due to the high variability of compounds that might be found in samples, test interferences caused by matrix effects cannot be completely excluded.

Mistakes in handling the test can cause errors. Possible sources for such errors include: inadequate storage conditions of the test kit, incorrect pipetting sequence or inaccurate volumes of the reagents, too long or too short incubation times during the immune and/or substrate reaction, extreme temperatures (lower than 10°C or higher than 30°C) during the test performance.

The Abraxis 2,4-D ELISA kit provides screening results. As with any analytical technique (GC, HPLC, etc.), samples requiring some regulatory action should be confirmed by an alternative method.

### A. Reagents and Materials Provided

1. Microtiter plate (12 X 8 strips) coated with a secondary antibody, in a resealable aluminum pouch
2. 2,4-D Calibrators/Standards (7): 0, 2, 5, 10, 20, 40, 80 ng/mL (ppb), 1 mL each
3. Antibody Solution (mouse anti-2,4-D), 6 mL
4. 2,4-D-HRP Conjugate Solution, 6 mL
5. Wash Solution (5X) Concentrate, 100 mL, must be diluted before use, see Test Preparation (Section C)
6. Sample Diluent, 25 mL
7. Substrate (Color) Solution (TMB), 16 mL
8. Stop Solution, 12 mL (handle with care)

### B. Additional Materials (not delivered with the test kit)

1. Micro-pipettes with disposable plastic tips (50-200  $\mu$ L)
2. Multi-channel pipette (50-250  $\mu$ L) or stepper pipette with disposable plastic tips (50-250  $\mu$ L)
3. Microtiter plate reader (wave length 450 nm)
4. Deionized or distilled water
5. Paper towels or equivalent absorbent material
6. Timer
7. Tape or parafilm

### C. Test Preparation

Micro-pipetting equipment and pipette tips for pipetting the standards and the samples are necessary. In order to equalize the incubation periods on the entire microtiter plate, a multi-channel pipette or a stepping pipette is recommended for adding the enzyme conjugate, antibody, substrate, and stop solutions. Please only use the reagents and standards from one package lot in one test, as they have been adjusted in combination.

1. Adjust the microtiter plate and the reagents to room temperature before use.
2. Remove the number of microtiter plate strips required from the aluminum pouch. The remaining strips are stored in the aluminum pouch and zip-locked closed. Store the remaining kit in the refrigerator (4-8°C).
3. The standard solutions, conjugate, antibody, substrate and stop solutions are ready to use and do not require any further dilutions.
4. Dilute the Wash Solution (5X) Concentrate at a ratio of 1:5. If using the entire bottle (100 mL), add to 400 mL of deionized or distilled water and mix thoroughly.
5. The stop solution must be handled with care as it contains diluted H<sub>2</sub>SO<sub>4</sub>.

### E. Working Scheme

The microtiter plate consists of 12 strips of 8 wells, which can be used individually for the test. The standards must be run with each test. Never use the values of standards which have been determined in a test performed previously.

Std 0-Std 6: Standards  
(0; 2; 5; 10; 20; 40; 80 ppb)

Samp1, Samp2, etc.: Samples

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 0	Std 4	Samp2									
B	Std 0	Std 4	Samp2									
C	Std 1	Std 5	etc.									
D	Std 1	Std 5	etc.									
E	Std 2	Std 6										
F	Std 2	Std 6										
G	Std 3	Samp1										
H	Std 3	Samp1										

### F. Assay Procedure

1. Add 50  $\mu$ L of the **calibrator/standard solutions or samples** into the wells of the test strips according to the working scheme given. Analysis in duplicate or triplicate is recommended.
2. Add 50  $\mu$ L of **enzyme conjugate solution** to the individual wells successively using a multi-channel pipette or a stepping pipette.
3. Add 50  $\mu$ L of **antibody solution** to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Be careful not to spill the contents.
4. Incubate the strips for 60 minutes at room temperature.
5. Remove the covering and decant the contents of the wells into a sink. Wash the strips **three times** using the **diluted washing buffer solution**. Please use at least a volume of 250  $\mu$ L of washing buffer for each well in each washing step. Remaining buffer in the wells should be removed by patting the inverted plate dry on a stack of paper towels.
6. Add 150  $\mu$ L of **substrate (color) solution** to the wells. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a circular motion on the benchtop for 30 seconds. Be careful not to spill the contents. Incubate the strips for 20 minutes at room temperature. Protect the strips from direct sunlight.
7. Add 100  $\mu$ L of **stop solution** to the wells in the same sequence as for the substrate solution.
8. Read the absorbance at 450 nm using a microplate ELISA photometer within 15 minutes after the addition of stopping solution.

### G. Evaluation

The evaluation of the ELISA can be performed using commercial ELISA evaluation programs such as 4-Parameter (preferred) or Logit/Log. For a manual evaluation, calculate the mean absorbance value for each of the standards. Calculate the %B/B<sub>0</sub> for each standard by dividing the mean absorbance value for each standard by the Zero Standard (Standard 0) mean absorbance. Construct a standard curve by plotting the %B/B<sub>0</sub> for each standard on the vertical linear (y) axis versus the corresponding 2,4-D concentration on the horizontal logarithmic (x) axis on graph paper. %B/B<sub>0</sub> for samples will then yield levels in ppb (or ng/mL) of 2,4-D by interpolation using the standard curve. Results can also be obtained by using a spreadsheet macro available from Abraxis upon request.

The concentrations of the samples are determined using the standard curve run with each test. Sample extracts showing a lower concentration of 2,4-D than standard 1 (2 ppb) should be reported as containing < 2 ppb of 2,4-D. Samples showing a higher concentration than standard 6 (80 ppb) must be diluted further with the provided sample diluent and re-analyzed.

Semi-quantitative results can be derived by simple comparison of the sample absorbances to the absorbances of the calibrators. Samples with lower absorbances than a calibrator will have concentrations of 2,4-D greater than the concentration of that calibrator. Samples which have higher absorbances than a calibrator will have concentrations of 2,4-D less than that calibrator.

### H. Recoveries


Surface water samples from various sources were spiked with various levels of 2,4-D and assayed using the Abraxis 2,4-D plate ELISA. The following results were obtained:

2,4-D Added (ppb)	Mean Recovery (ppb)	S.D. (ppb)	% Recovery
3.75	3.808	0.563	102%
7.5	7.480	0.679	100%
15	14.228	1.168	95%
30	28.752	3.124	96%
Average			98%

# 2,4-D Plate, Detailed ELISA Procedure


## 1. Addition of Standards, Samples

Add 50  $\mu$ L of calibrators or sample into the wells of the test strips according to the working scheme given. Be sure to use a clean pipet tip for each.

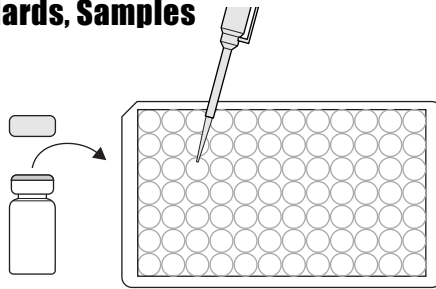


## 2. Addition of Enzyme Conjugate

Add 50  $\mu$ L of the enzyme conjugate to the individual wells successively using a multi-channel pipette or a stepping pipette.

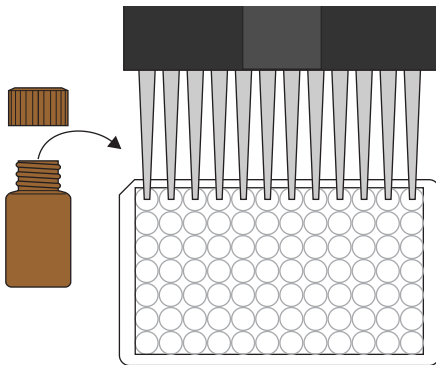


## 3. Addition of Antibody Solution

Add 50  $\mu$ L of the antibody solution to the individual wells successively using a multi-channel pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 60 min. at room temperature.

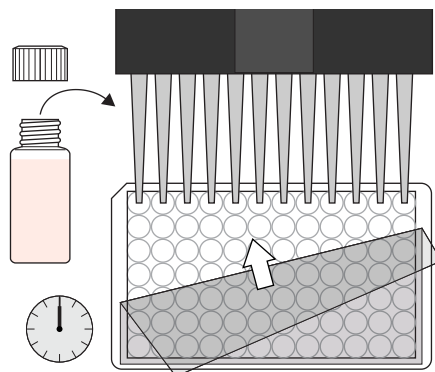


## 4. Washing of Plates

After incubation, remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips three times with a multi-channel pipette or wash bottle using the diluted 1X washing buffer solution. Please use at least a volume of 250  $\mu$ L of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels.

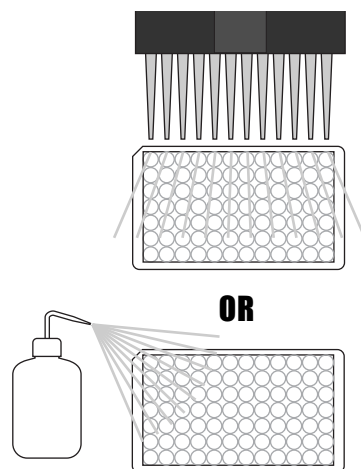


## 5. Addition of Substrate/Color Solution

Add 150  $\mu$ L of substrate/color solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 20 min. at room temperature.

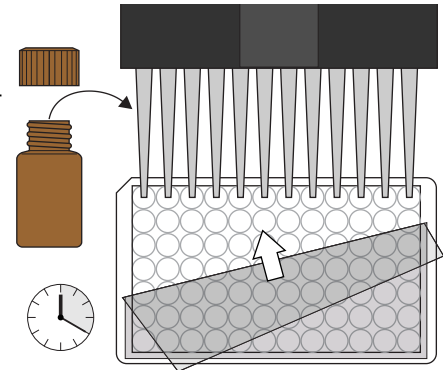


## 6. Addition of Stopping Solution

Add 100  $\mu$ L of stop solution to the wells in the same sequence as for the substrate solution using a multi-channel pipette or a stepping pipette.

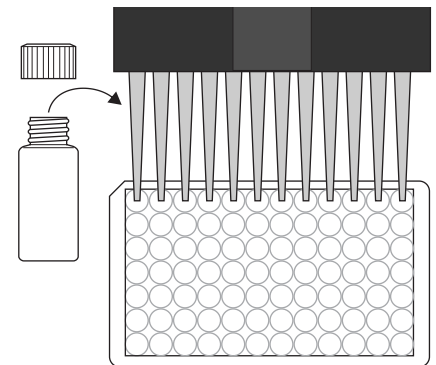

## 7. Measurement of Color

Read the absorbance at 450 nm using a microplate ELISA reader. Calculate results.

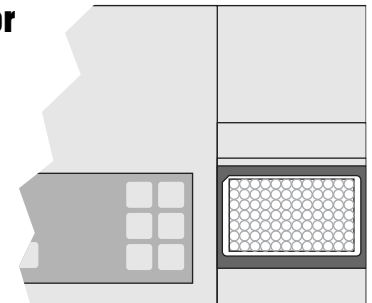

India Contact:


**Life Technologies (India) Pvt. Ltd.**

306, Aggarwal City Mall, Road No. 44, Pitampura, Delhi - 110034, India  
Mobile: +91-98105-21400, Tel: +91-11-42208000, 8111, 8222, Fax: +91-11-42208444  
Email: customerservice@lifetechindia.com, [www.atzlabs.com](http://www.atzlabs.com); [www.lifetechindia.com](http://www.lifetechindia.com)

# 2,4-D Plate, Concise ELISA Procedure


## 1. Addition of Standards, Samples

Add 50 uL of calibrators or diluted sample extracts.

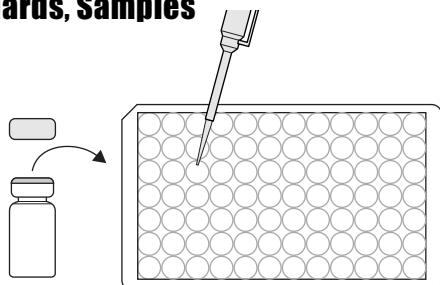


## 2. Addition of Enzyme Conjugate

Add 50 uL of enzyme conjugate.

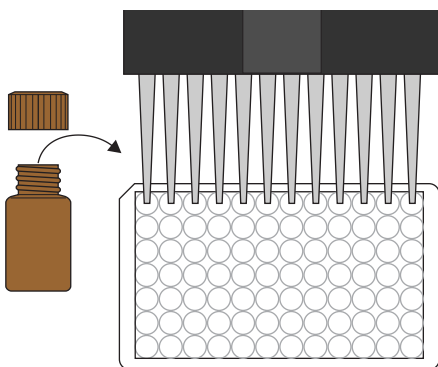


## 3. Addition of Antibody Solution

Add 50 uL of the antibody solution. Cover and mix for 30 seconds by rotating on benchtop. Incubate for 60 minutes at room temperature.

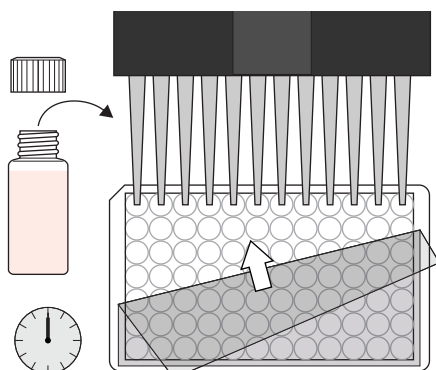


## 4. Washing of Plates

Wash the plates three times with 250 uL of diluted 1X washing buffer.

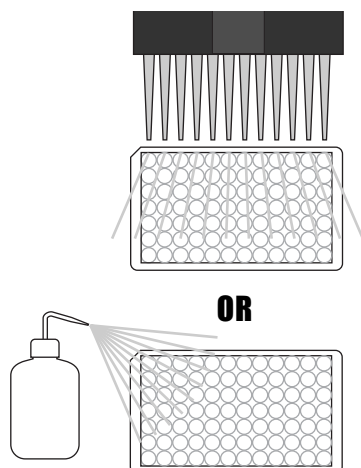


## 5. Addition of Substrate/Color Solution

Add 150 uL of substrate/color solution. Incubate 20 minutes at room temperature and away from direct sunlight.

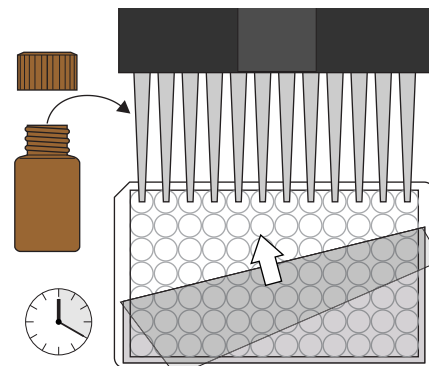


## 6. Addition of Stopping Solution

Add 100 uL of stop solution.

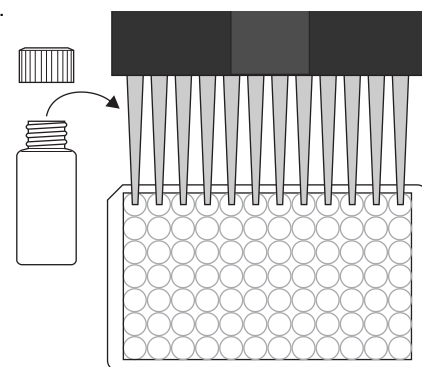

## 7. Measurement of Color

Measure color at 450 nm. Calculate results.

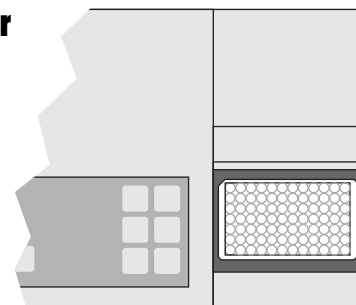

India Contact:

**Life Technologies (India) Pvt. Ltd.**

306, Aggarwal City Mall, Road No. 44, Pitampura, Delhi - 110034, India

Mobile: +91-98105-21400, Tel: +91-11-42208000, 8111, 8222, Fax: +91-11-42208444

Email: [customerservice@lifetechindia.com](mailto:customerservice@lifetechindia.com), [www.atzlabs.com](http://www.atzlabs.com); [www.lifetechindia.com](http://www.lifetechindia.com)

# Safety Data Sheet

## Section 1: Product and Company Identification

### 1.1 Product Identifiers:

**Product Name:** 2,4-D Plate Kit

**Product Code:** 54003A

**1.2 Identified Use:** Determination of 2,4-D in samples. **Restrictions on Use:** For research use only.

**1.3 Company:** Abraxis, Inc., 124 Railroad Drive, Warminster, PA 18974 USA, [info@abraxiskits.com](mailto:info@abraxiskits.com) +1(215) 357-3911, FAX +1(215) 357-5232

**1.4 Emergency Telephone Number:** +1(215) 357-3911

## Section 2: Hazard(s) Identification

### 2.1 Classification of the mixture:

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

Flammable liquids (Category 2), H225 Highly flammable liquid and vapor

Acute toxicity, Oral (Category 3), H301 Toxic if swallowed

Acute toxicity, Inhalation (Category 3), H331 Toxic if inhaled

Acute toxicity, Dermal (Category 3), H311 Toxic in contact with skin

Specific target organ toxicity - single exposure (Category 1), H370 Causes damage to organs

HMIS Rating: Health hazard: 2, Chronic Health Hazard: \*, Flammability: 3, Physical Hazard 0

NFPA Rating: Health hazard: 2, Fire Hazard: 3, Reactivity Hazard: 0

### 2.2 GHS Label elements, including precautionary statements:

Pictogram(s)



Signal word: Danger

Hazard statement(s):

H225 Highly flammable liquid and vapor.

H301 + H311 + H331 Toxic if swallowed, in contact with skin, or if inhaled

H370 Causes damage to organs.

Precautionary statement(s):

P210 Keep away from heat/sparks/open flames/hot surfaces. No smoking.

P233 Keep container tightly closed.

P240 Ground/bond container and receiving equipment.

P241 Use explosion-proof electrical/ventilating/lighting equipment.

P242 Use only non-sparking tools.

P243 Take precautionary measures against static discharge.

P260 Do not breathe dust/fume/gas/mist/vapors/ spray.

P264 Wash skin thoroughly after handling.

P270 Do not eat, drink or smoke when using this product.

P271 Use only outdoors or in a well-ventilated area.

P280 Wear protective gloves/eye protection/face protection.

P301 + P310 + P330 IF SWALLOWED: Immediately call a POISON CENTER or doctor/physician. Rinse mouth.

P303 + P361 + P353 IF ON SKIN (or hair): Take off immediately all contaminated clothing. Rinse skin with water/shower.

P304 + P340 + P311 IF INHALED: Remove person to fresh air and keep comfortable for breathing. Call a POISON CENTER or doctor/physician.

P307 + P311 If exposed: Call a POISON CENTER or doctor/physician.

P362 Take off contaminated clothing and wash before reuse.

P370 + P378 In case of fire: Use dry sand, dry chemical or alcohol-resistant foam to extinguish.

P403 + P233 Store in a well-ventilated place. Keep container tightly closed.

P403 + P235 Store in a well-ventilated place. Keep cool.

P405 Store locked up.

P501 Dispose of contents/ container to an approved waste disposal plant.

**2.3 Hazards not otherwise classified (HNOC) or not covered by GHS:** None known.

**2.4 Unknown acute toxicity:** None known.

## Section 3: Composition / Information on Ingredients

**3.2 Mixtures:** Mixture of the hazardous substance(s) listed below, with nonhazardous additions.

Hazardous component(s):

Name and Synonym(s): Methyl alcohol, MeOH, Methanol      Formula: CH<sub>4</sub>O      Molecular weight: 32.04 g/mol

CAS No.: 67-56-1      EC-No.: 200-659-6

Classification: Flammable Liquid 2, Acute Toxicity 3; STOT SE 1; H225, H301 + H311 + H331, H370

Percentage in Mixture: 4 %

For full text of H-Statements mentioned in this Section, see Section 2.

#### Section 4: First Aid Measures

**4.1 Description of first aid measures:** Consult a physician. Show this safety data sheet to the doctor in attendance. Move out of dangerous area.

**If inhaled:** If breathed in, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

**In case of skin contact:** Wash off with soap and plenty of water. Take victim immediately to hospital. Consult a physician.

**In case of eye contact:** Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

**If swallowed:** Do NOT induce vomiting. Never give anything by mouth to an unconscious person. Rinse mouth with water. Consult a physician.

**4.2 Most important symptoms and effects, both acute and delayed:** The most important known symptoms and effects are described in the labelling (see section 2.2) and/or in section 11

**4.3 Indication of any immediate medical attention and special treatment needed:** No data available. Treat symptomatically.

#### Section 5: Fire-fighting Measures

**5.1 Suitable extinguishing media:** Dry powder or sand      **Unsuitable extinguishing media:** Do NOT use water jet

**5.2 Special hazards arising from the substance or mixture:** Carbon oxides

**5.3 Advice for firefighters:** Wear self-contained breathing apparatus for fire-fighting if necessary.

**5.4 Further information:** Use water spray to cool unopened containers.

#### Section 6: Accidental Release Measures

**6.1 Personal precautions, protective equipment and emergency procedures:** Use personal protective equipment (see section 8). Avoid dust formation. Avoid breathing vapors, mist, dust, or gas. Ensure adequate ventilation. Remove all sources of ignition. Evacuate personnel to safe areas.

**6.2 Environmental precautions:** Prevent further leakage or spillage if safe to do so. Do not let product enter drains. Discharge into the environment must be avoided.

**6.3 Methods and materials for containment and cleaning up:** Contain spillage. Solids (if applicable): Pick up and arrange disposal without creating dust. Sweep up and shovel. Liquids (if applicable): Absorb with non-combustible liquid-binding material (sand, earth, diatomite, vermiculite). Keep in suitable, closed containers for disposal.

**6.4 Reference to other sections:** For information on safe handling see section 7.

For information on personal protection see section 8.

For information on disposal see section 13.

#### Section 7: Handling and Storage

**7.1 Precautions for safe handling:** See section 2. Avoid inhalation of vapors or mist, and avoid contact with skin and eyes. Wear appropriate personal protective equipment. Use explosion-proof equipment. Keep away from sources of ignition. Do not eat, drink, or smoke in work area. Take measures to prevent the buildup of electrostatic charge.

**7.2 Precautions for safe storage:** Keep container(s) tightly closed in a dry, well-ventilated place. Protect from physical damage. Opened containers must be carefully resealed and kept upright to prevent leakage. See label or product insert for appropriate storage temperature and additional specific information. Storage class (TRGS 510): Flammable liquids.

**7.3 Specific end use(s):** Other than use(s) specified in section 1, no other uses are stipulated.

#### Section 8: Exposure Controls / Personal Protection

**8.1 Control parameters:**

**Component(s) with workplace control parameters**

Methanol, CAS No. 67-56-1

Value	Control parameters	Basis
TWA	200.000000 ppm	USA. ACGIH Threshold Limit Values (TLV)
Headache Nausea Dizziness Eye damage		

Substances for which there is a Biological Exposure Index or Indices (see BEI section) Danger of cutaneous absorption		
STEL	250.000000 ppm	USA. ACGIH Threshold Limit Values (TLV)
Headache Nausea Dizziness Eye damage Substances for which there is a Biological Exposure Index or Indices (see BEI section) Danger of cutaneous absorption		
TWA	200.000000 ppm; 260.000000 mg/m <sup>3</sup>	USA. NIOSH Recommended Exposure Limits
Potential for dermal absorption		
ST	250.000000 ppm; 325.000000 mg/m <sup>3</sup>	USA. NIOSH Recommended Exposure Limits
Potential for dermal absorption		
TWA	200.000000 ppm; 260.000000 mg/m <sup>3</sup>	USA. Occupational Exposure Limits; (OSHA) - Table Z-1 Limits for Air Contaminants
The value in mg/m <sup>3</sup> is approximate		
TWA	200 ppm; 260 mg/m <sup>3</sup>	USA. NIOSH Recommended Exposure Limits
Potential for dermal absorption		
ST	250 ppm; 325 mg/m <sup>3</sup>	USA. NIOSH Recommended Exposure Limits
Potential for dermal absorption		
TWA	200 ppm; 260 mg/m <sup>3</sup>	USA. Occupational Exposure Limits; (OSHA) - Table Z-1 Limits for Air Contaminants
The value in mg/m <sup>3</sup> is approximate		
STEL	250 ppm; 325 mg/m <sup>3</sup>	USA. OSHA - TABLE Z-1 Limits for Air Contaminants - 1910.1000
Skin notation		
TWA	200 ppm; 260 mg/m <sup>3</sup>	USA. OSHA - TABLE Z-1 Limits for Air Contaminants - 1910.1000
Skin notation		

#### Biological occupational exposure limits

Methanol, CAS No. 67-56-1

Parameters	Value	Biological specimen	Basis
Methanol	15.0000 mg/l	Urine	ACGIH – Biological Exposure Indices (BEI)
End of shift (As soon as possible after exposure ceases)			

#### Derived No Effect Level (DNEL)

Methanol, CAS No. 67-56-1

Application area	Exposure routes	Health effect	Value
Workers	Skin contact	Long-term systemic effects, Acute systemic effects	40mg/kg BW/d
Consumers	Skin contact	Long-term systemic effects, Acute systemic effects	8mg/kg BW/d
Consumers	Ingestion	Long-term systemic effects, Acute systemic effects	8mg/kg BW/d
Workers	Inhalation	Acute systemic effects, Acute local effects, Long-term systemic effects, Long-term local effects	260 mg/m <sup>3</sup>
Consumers	Inhalation	Acute systemic effects, Acute local effects, Long-term systemic effects, Long-term local effects	50 mg/m <sup>3</sup>

#### Predicted No Effect Concentration (PNEC)

Methanol, CAS No. 67-56-1

Compartment	Value
Soil	23.5 mg/kg
Marine water	15.4 mg/l
Fresh water	154 mg/l
Fresh water sediment	570.4 mg/kg
Onsite sewage treatment plant	100 mg/kg

## 8.2 Exposure controls:

**Appropriate engineering controls:** Provide adequate ventilation. Handle in accordance with good industrial hygiene and safety practice. Wash hands before breaks and at the end of workday. Keep away from food and beverages.

### Personal protective equipment

**Eye protection:** Use equipment for eye protection tested and approved under appropriate government standards such as NIOSH (US) or EN 166 (EU).

**Skin protection:** Handle with chemical resistant gloves. Gloves must be inspected prior to use. Use proper glove removal technique (without touching glove's outer surface) to avoid skin contact with this product. Dispose of contaminated gloves after use in accordance with applicable laws and good laboratory practices. Wash and dry hands.

**Respiratory protection:** Use a chemical fume hood or approved respiratory protection equipment.

**Body protection:** Lightweight, protective clothing to prevent skin exposure.

## Section 9: Physical and Chemical Properties

### 9.1 Information on basic physical and chemical properties of mixture

**Appearance:** Multiple

**Odor:** Characteristic

**Odor Threshold:** No data available

**pH:** Multiple

**Melting point/freezing point:** No data available

**Initial boiling point and boiling range:** No data available

**Flash point:** No data available

**Evaporation rate:** No data available

**Flammability (solid, gas):** No data available

**Upper/lower flammability or explosive limits:** No data available

**Vapor pressure:** No data available

**Vapor density:** No data available

**Relative density:** No data available

**Water solubility:** Various

**Partition coefficient: n-octanol/water:** No data available

**Auto-ignition temperature:** Not applicable

**Decomposition temperature:** No data available

**Viscosity:** No data available

**Explosive properties:** No data available

**Oxidizing properties:** No data available

**9.2 Other information:** No data available

## Section 10: Stability and Reactivity

**10.1 Reactivity:** No data available

**10.2 Chemical stability:** Stable under recommended storage conditions.

**10.3 Possibility of hazardous reactions:** No data available

**10.4 Conditions to avoid:** Keep away from open flame, hot surfaces, heat sources, and sources of ignition.

**10.5 Incompatible materials:** Acid chlorides, acid anhydrides, strong oxidizing agents, alkali metals, reducing agents, acids, peroxides

**10.6 Hazardous decomposition products:** No data available. In the event of fire: see section 5.

## Section 11: Toxicological Information

### 11.1 Information on toxicological effects

To the best of our knowledge, the chemical, physical, and toxicological properties of this product have not been thoroughly investigated.

**Acute toxicity (Methanol, CAS No. 67-56-1):**

**Inhalation** LC50 Inhalation - Rat - 4 h - 128.2 mg/l; LC50 Inhalation - Rat - 6 h - 87.6 mg/l; LD50 Dermal - Rabbit - 17,100 mg/kg

**Ingestion** LDLO Oral - Human - 143 mg/kg (Lungs, Thorax, or Respiration:Dyspnea. Ingestion may cause gastrointestinal irritation, nausea, vomiting and diarrhea); LD50 Oral - Rat - 1,187 - 2,769 mg/kg

**Skin contact** Rabbit skin—no irritation

**Eye contact** Rabbit eye—no irritation

**Respiratory or skin sensitization** Maximization Test (GPMT)(OECD Test Guideline 406)--Guinea pig--does not cause skin sensitization

**Aspiration hazard** No data available

**Mutagenicity (Methanol, CAS No. 67-56-1):** Ames test (*S. typhimurium*)--Result: negative; *in vitro* assay (fibroblasts)--Result: negative; *in vivo* mammalian bone-marrow cytogenetic test, chromosomal analysis (mouse, male and female)--Result: negative

**Carcinogenicity:**

IARC: No component of this product present at levels greater than or equal to 0.1% is identified as probable, possible or confirmed human carcinogen by IARC.

ACGIH: No component of this product present at levels greater than or equal to 0.1% is identified as a carcinogen or potential carcinogen by ACGIH.

NTP: No component of this product present at levels greater than or equal to 0.1% is identified as a known or anticipated carcinogen by NTP.

OSHA: No component of this product present at levels greater than or equal to 0.1% is identified as a carcinogen or potential carcinogen by OSHA.

**Teratogenicity:** No data available

**Reproductive/fertility toxicity:** Damage to fetus not classifiable

**Specific target organ toxicity, single exposure** (Methanol, CAS No. 67-56-1): Causes damage to organs

**Specific target organ toxicity, repeated exposure:** The substance or mixture is not classified as specific target organ toxicant, repeated exposure.

**Additional information** (Methanol, CAS No. 67-56-1): RTECS: PC1400000 Effects due to ingestion may include headache, dizziness, drowsiness, metabolic acidosis, coma, seizures. Methanol may be fatal or cause blindness if swallowed. Stomach - Irregularities - Based on Human Evidence

**Section 12: Ecological Information**

**12.1 Toxicity:** No data available

**12.2 Persistence and degradability:** Readily biodegradable

**12.3 Bioaccumulative potential:** No data available

**12.4 Mobility in soil:** No data available

**12.5 Results of PBT and vPvB assessment:** No data available

**12.6 Other adverse effects:** An environmental hazard cannot be excluded in the event of unprofessional handling or disposal.

**Section 13: Disposal Considerations****13.1 Waste treatment methods**

**Product:** All waste must be handled and disposed according to local, state, and federal regulations. Avoid disposing large volumes in sewer.

**Contaminated packaging:** All waste must be handled and disposed according to local, state, and federal regulations.

Refer to sections 7 and 8 for safe handling guidance.

**Section 14: Transport Information**

DOT, Land Transport ADR/RID (cross-border), Maritime Transport IMDG, Air Transport ICAO-TI and IATA-DGR

**UN Number:** 3316

**UN Proper shipping name:** Chemical Kit, (contains Methanol)

**Transport hazard class(es):** 9

**Packing group:** III

**Environmental hazard:** See section 12

**Bulk transport:** Excepted/Limited quantity

**Special considerations:** See section 7 for handling

**Section 15: Regulatory Information**

**EU Regulations, Hazard Symbol(s):** Methanol: T (Toxic), F (Flammable)

**Safety Phrases:**

Methanol: S 7 / 16 / 36 / 37 / 45, Keep container tightly closed. Keep away from sources of ignition, no smoking. Wear suitable protective clothing and gloves. In case of accident or if you become ill, seek medical advice immediately (show product label).

**SARA Title III, Section 313 Components:** Methanol, CAS No. 67-56-1

**SARA 311/312 Hazards:** Methanol, CAS No. 67-56-1: Fire Hazard, Acute Health Hazard, Chronic Health Hazard

**State Right-to-Know**

Massachusetts: Methanol, CAS No. 67-56-1

Pennsylvania: Methanol, CAS No. 67-56-1

New Jersey: Methanol, CAS No. 67-56-1

California Prop. 65 Components: WARNING: This product contains a chemical known to the State of California to cause birth defects or other reproductive harm. Methanol, CAS No. 67-56-1

**Section 16: Other information**

This information is based on our present knowledge. While Abraxis , Inc. believes that the data contained herein are factual and the opinions expressed represent a best effort to present accurate information, the data are not to be taken as a warranty or representation for which Abraxis , Inc. assumes legal responsibility. The information shall not be taken as being all-inclusive and is to be used only as a guide. The data are offered solely for the user's consideration, investigation, and verification. These suggestions should not be confused with either state, municipal, or insurance requirements, or with national safety codes and constitute no warranty. Any use of these data and information must be determined by the user to be in accordance with applicable federal, state, and local regulations.

All materials and mixtures may present unknown hazards and should be used with caution. Since Abraxis , Inc. cannot control the methods, volumes, or conditions of use of this product, Abraxis , Inc. shall not be held liable for any damages or losses resulting from the handling or from contact with the product as described herein. An individual technically qualified to handle potentially hazardous chemicals must supervise the use of this material. This product is sold for research use only. It is not for any human or animal therapeutic or clinical diagnostic use.

**Date this SDS was prepared:** 5/20/2016

**Version:** 3

**Changes from previous version:** Abraxis, LLC changed to Abraxis, Inc.